

Incontinence shouldn't be inevitable


The Biodesign Anal Fistula Plug minimizes the risk of postoperative incontinence and provides a biologic, minimally invasive option for sphincter-sparing fistula repair.¹

>90%

patient, doctor

SATISFACTION

with operative outcomes²

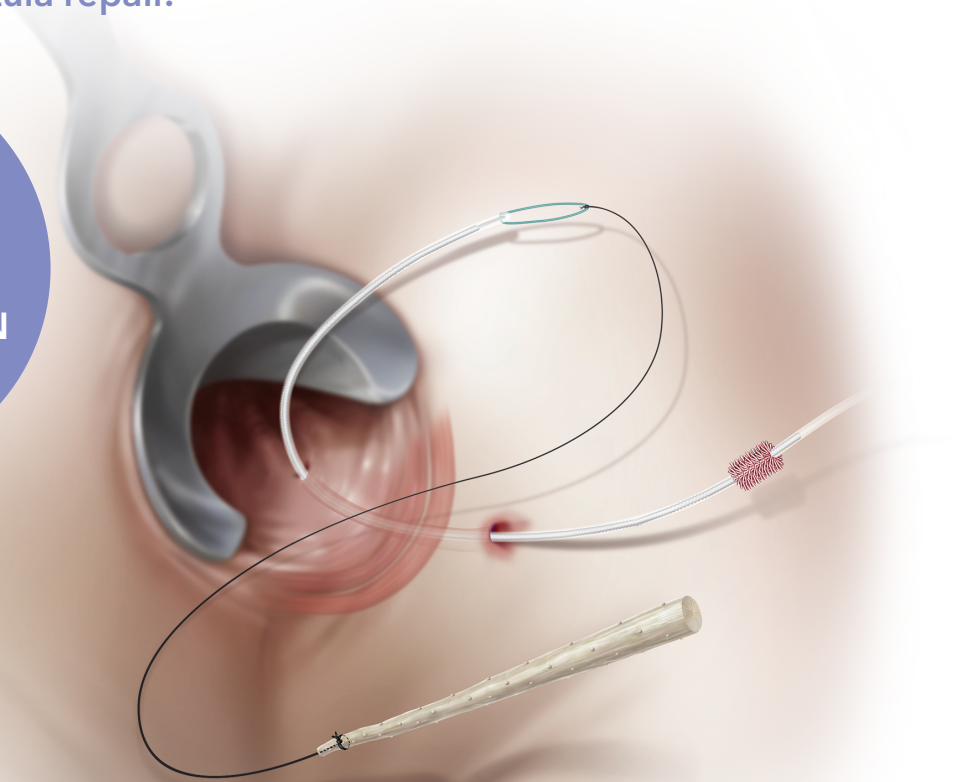


Biodesign®
BIOLOGIC GRAFT PORTFOLIO

1. van Koperen PJ, Bemelman WA, Gerhards MF, et al. The anal fistula plug treatment compared with the mucosal advancement flap for cryptoglandular high transsphincteric perianal fistula: a double-blinded multicenter randomized trial. *Dis Colon Rectum*. 2011;54(4):387-393. Note: The name of our product has changed since this trial was published.
2. Chen ZW, Zheng Y, Zhao R, Wang ZJ. Treatment of anal fistula using a decellularized porcine small intestinal submucosa plug: A non-inferiority trial. *Medicine*. 2022;101(29):e29110.

Biodesign biologics become you™

No permanent material left behind³

Biodesign biologic grafts are derived from **small intestinal submucosa (SIS)**, a naturally occurring, **intact extracellular matrix**. SIS acts as a scaffold that allows host cells to infiltrate and **remodel into vascularized tissue**, leaving **no permanent material in the patient's body**.³

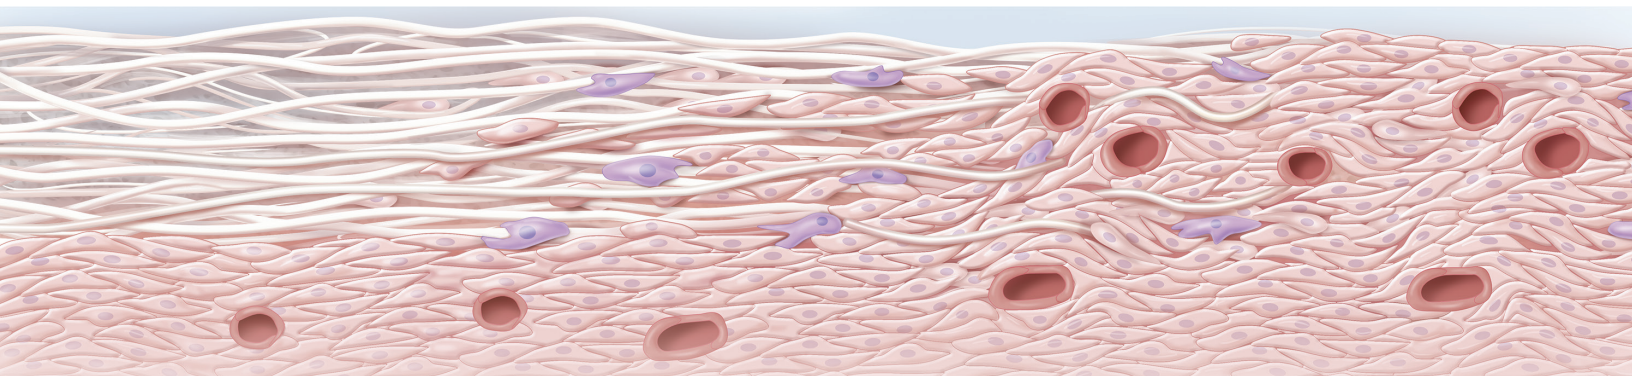

SIS scaffold ➔ Infiltration of host cells ➔ Vascularized tissue

Product information

Biodesign Anal Fistula Plug

For implantation to reinforce soft tissue where a rolled configuration is required, for repair of anorectal fistulas

Order Number	Reference Part Number	Size cm
G53614	C-AFPS-0.6X9.5	0.6 x 9.5

Product features

- Manufactured in the US
- Biologic xenograft made from porcine SIS
- Non-cross-linked, non-dermis
- Easily hydrated in the operating room
- No special orientation or sidedness
- Off-the-shelf product that does not require special storage
- Does not require AATB tissue tracking
- MRI safe

3. Franklin ME Jr, Trevino JM, Portillo G, Vela I, Glass JL, Gonzalez JJ. The use of porcine small intestinal submucosa as a prosthetic material for laparoscopic hernia repair in infected and potentially contaminated field: Long-term follow-up. *Surg Endosc*. 2008;22(9):1941-1946.

IMPORTANT RISK INFORMATION

As with all implantable xenografts, risks exist. Scan the QR code for detailed product information, including a link to the Instructions for Use, which contains the indication statement, contraindications, precautions, and potential complications.

