

Incontinence shouldn't be inevitable.


Biodesign fistula plugs minimize the risk of postoperative incontinence and provide biologic, minimally invasive options for sphincter-sparing fistula repair.¹

>90%

patient, doctor


SATISFACTION

with operative outcomes²

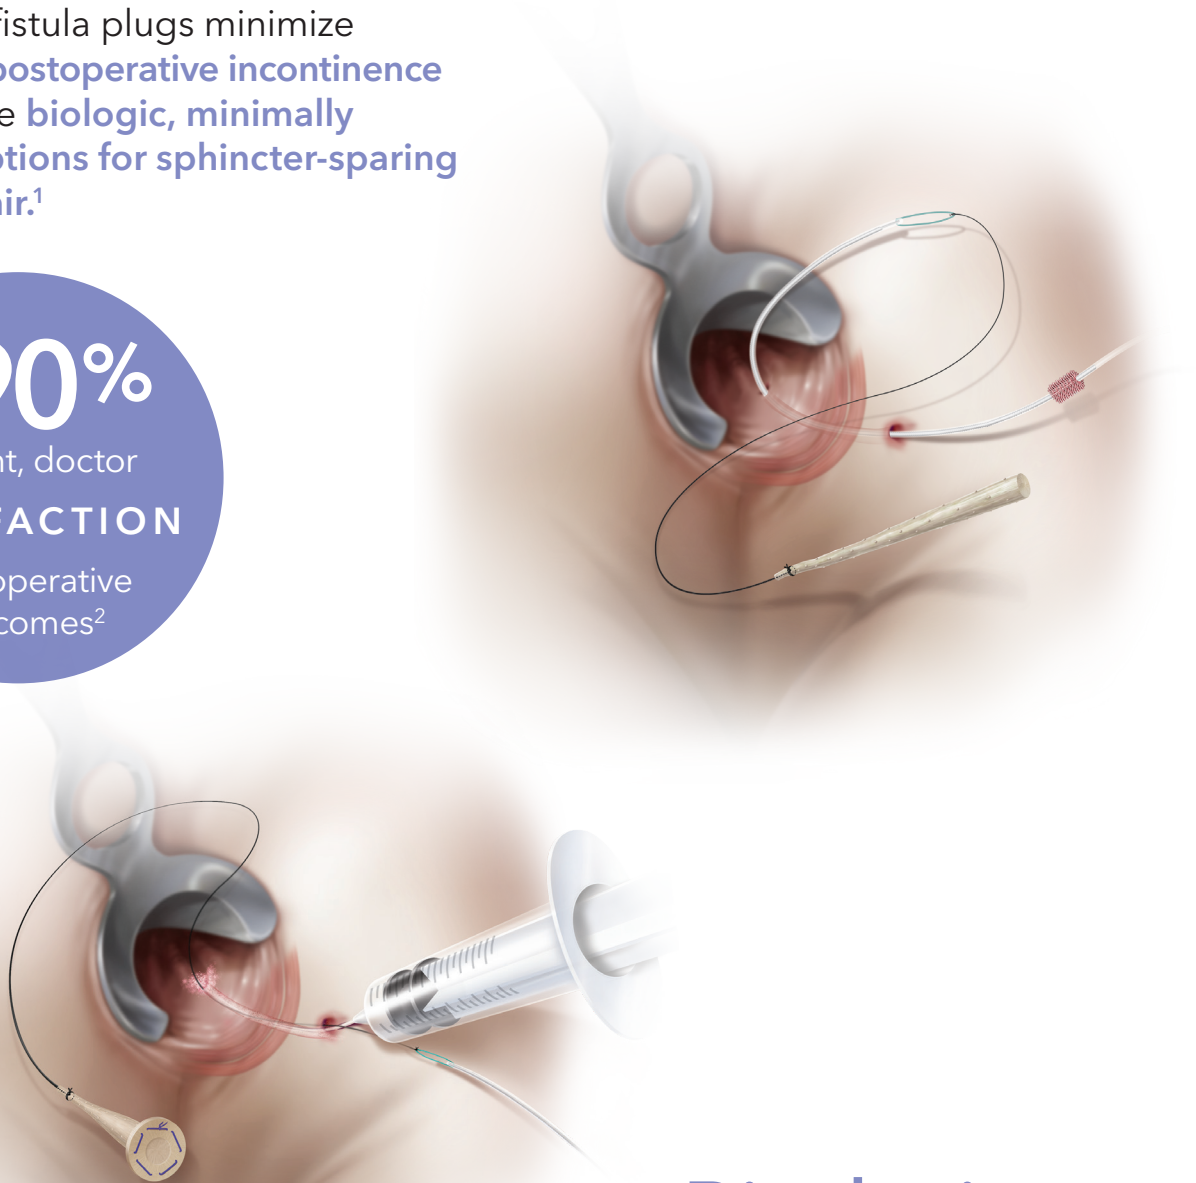

Biodesign[®]
BIOLOGIC GRAFT PORTFOLIO

1. van Koperen PJ, Bemelman WA, Gerhards MF, et al. The anal fistula plug treatment compared with the mucosal advancement flap for cryptoglandular high transsphincteric perianal fistula: a double-blinded multicenter randomized trial. *Dis Colon Rectum*. 2011;54(4):387-393. Note: The name of our product has changed since this trial was published.
2. Chen ZW, Zheng Y, Zhao R, Wang ZJ. Treatment of anal fistula using a decellularized porcine small intestinal submucosa plug: A non-inferiority trial. *Medicine*. 2022;101(29):e29110.

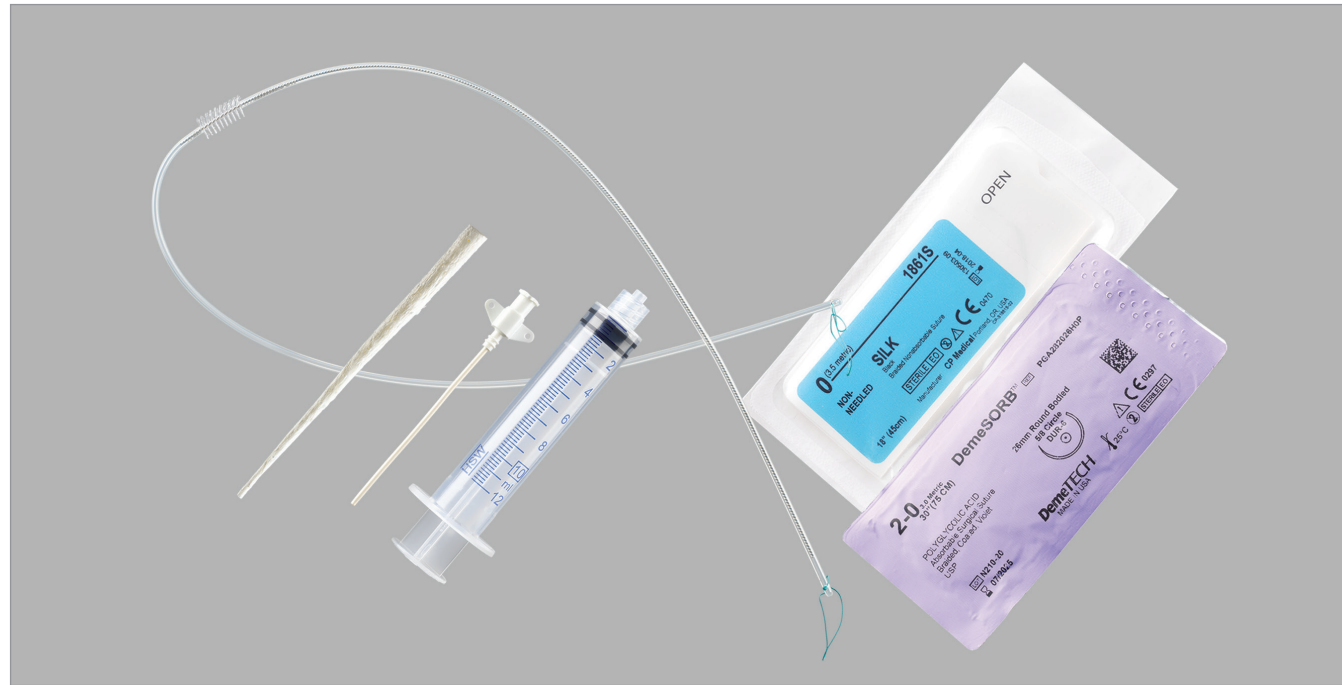

Product information

Biodesign Anal Fistula Plug Set

Used for implantation to reinforce soft tissue where a rolled configuration is required, for repair of anorectal fistulas

Order Number	Reference Part Number	Size cm
G53614	C-AFPS-0.6X9.5	0.6 x 9.5


Each plug set includes:

- Biodesign Anal Fistula Plug
- Cook® Fistula Brush
- Cook Irrigation Catheter
- 2-0 polyglycolic acid (PGA) absorbable suture with DUR-6 needle
- 0 silk nonabsorbable suture
- 10 ml Luer-lock syringe



IMPORTANT RISK INFORMATION

As with all implantable xenografts, risks exist. Scan the QR code for detailed product information, including a link to the Instructions for Use, which contains the indication statement, contraindications, precautions, and potential complications.

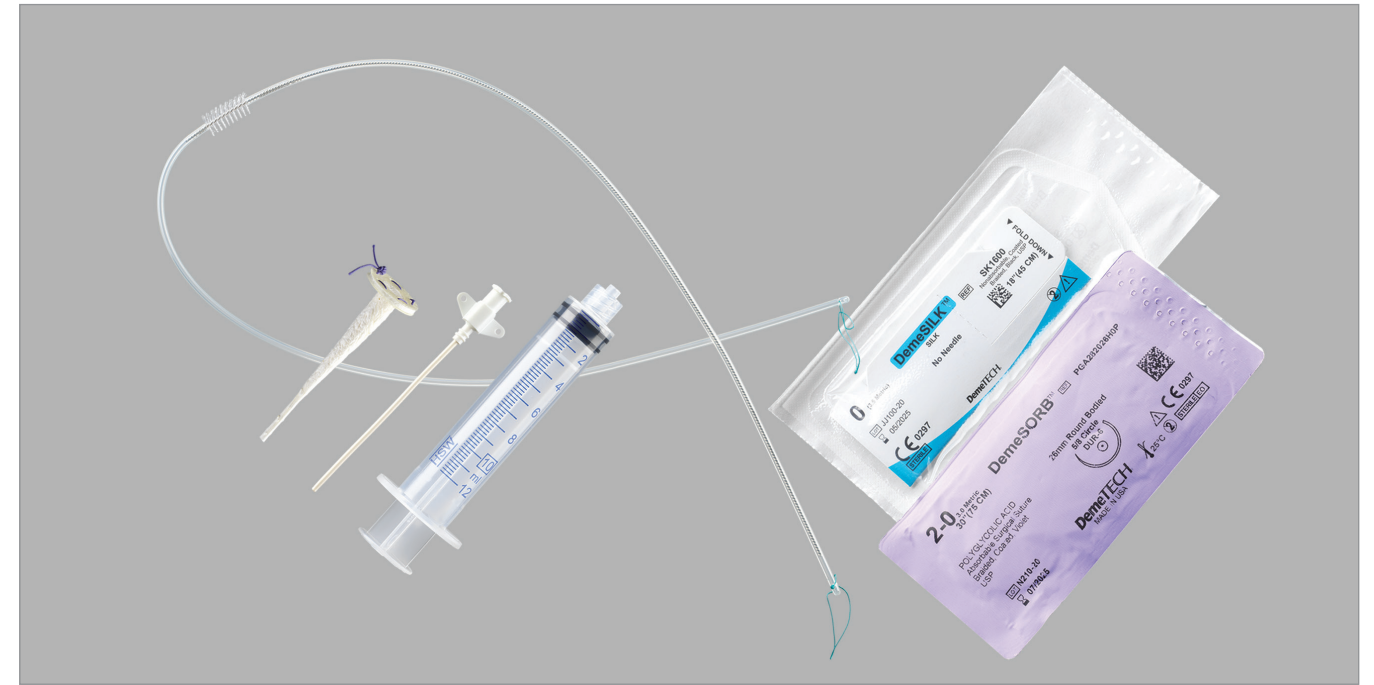

Product information

Biodesign Fistula Plug Set

Used for implantation to reinforce soft tissue for repair of recto-vaginal or anorectal fistulas

Order Number	Reference Part Number	Size cm
G54612	C-FPS-0.2	0.2
G54613	C-FPS-0.4	0.4
G54614	C-FPS-0.7	0.7

Each plug set includes:

- Biodesign Fistula Plug
- Cook Fistula Brush
- Cook Irrigation Catheter
- 2-0 polyglycolic acid (PGA) absorbable suture with DUR-6 needle
- 0 silk nonabsorbable suture
- 10 ml Luer-lock syringe




IMPORTANT RISK INFORMATION

As with all implantable xenografts, risks exist. Scan the QR code for detailed product information, including a link to the Instructions for Use, which contains the indication statement, contraindications, precautions, and potential complications.

Biodesign biologics become you™

No permanent material left behind³

Biodesign biologic grafts are derived from **small intestinal submucosa (SIS)**, a naturally occurring, **intact extracellular matrix**. SIS acts as a scaffold that allows host cells to infiltrate and **remodel into vascularized tissue**, leaving **no permanent material in the patient's body**.³

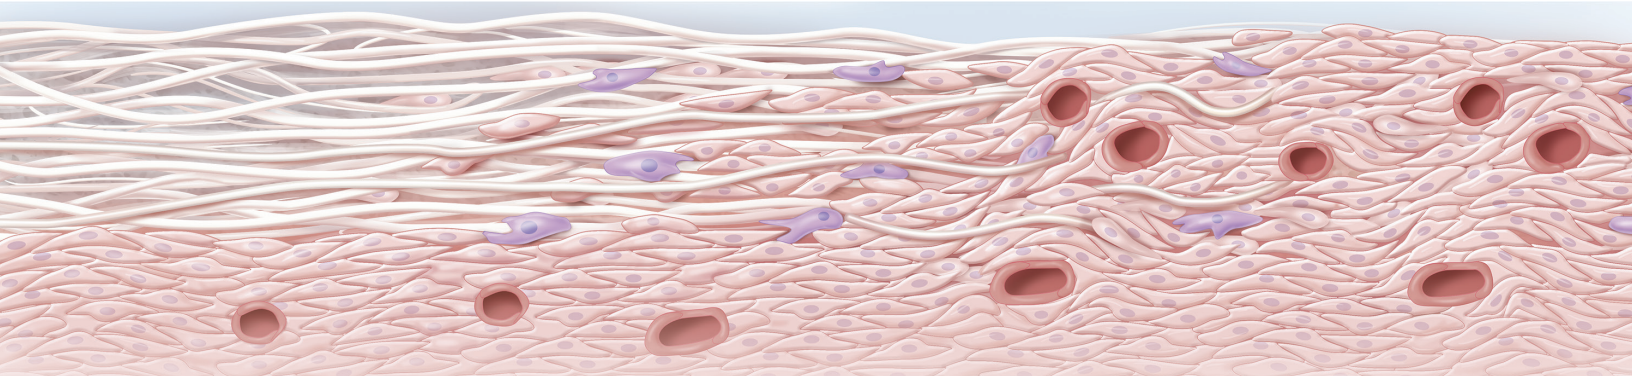

SIS scaffold → Infiltration of host cells → Vascularized tissue

Product features

- Manufactured in the US
- Biologic xenograft made from porcine SIS
- Non-cross-linked, non-dermis
- Easily hydrated in the operating room
- No special orientation or sidedness
- Off-the-shelf product that does not require special storage
- Does not require AATB tissue tracking
- MRI safe

3. Franklin ME Jr, Trevino JM, Portillo G, Vela I, Glass JL, Gonzalez JJ. The use of porcine small intestinal submucosa as a prosthetic material for laparoscopic hernia repair in infected and potentially contaminated field: Long-term follow-up. *Surg Endosc*. 2008;22(9):1941-1946.